

AID-173SHW

17.3" Medical PC

Quick Reference Guide

1st Ed – 06 January 2015

Copyright Notice

Copyright © 2015 Avalue Technology Inc., ALL RIGHTS RESERVED.

FCC Statement



THIS DEVICE COMPLIES WITH PART 15 FCC RULES. OPERATION IS SUBJECT TO THE FOLLOWING TWO CONDITIONS:

- (1) THIS DEVICE MAY NOT CAUSE HARMFUL INTERFERENCE.
- (2) THIS DEVICE MUST ACCEPT ANY INTERFERENCE RECEIVED INCLUDING INTERFERENCE THAT MAY CAUSE UNDESIRE OPERATION.

THIS EQUIPMENT HAS BEEN TESTED AND FOUND TO COMPLY WITH THE LIMITS FOR A CLASS "A" DIGITAL DEVICE, PURSUANT TO PART 15 OF THE FCC RULES.

THESE LIMITS ARE DESIGNED TO PROVIDE REASONABLE PROTECTION AGAINST HARMFUL INTERFERENCE WHEN THE EQUIPMENT IS OPERATED IN A COMMERCIAL ENVIRONMENT. THIS EQUIPMENT GENERATES, USES, AND CAN RADIATE RADIO FREQUENCY ENERGY AND, IF NOT INSTALLED AND USED IN ACCORDANCE WITH THE INSTRUCTION MANUAL, MAY CAUSE HARMFUL INTERFERENCE TO RADIO COMMUNICATIONS.

OPERATION OF THIS EQUIPMENT IN A RESIDENTIAL AREA IS LIKELY TO CAUSE HARMFUL INTERFERENCE IN WHICH CASE THE USER WILL BE REQUIRED TO CORRECT THE INTERFERENCE AT HIS OWN EXPENSE.

A Message to the Customer

Avalue Customer Services

Each and every Avalue's product is built to the most exacting specifications to ensure reliable performance in the harsh and demanding conditions typical of industrial environments. Whether your new Avalue device is destined for the laboratory or the factory floor, you can be assured that your product will provide the reliability and ease of operation for which the name Avalue has come to be known.

Your satisfaction is our primary concern. Here is a guide to Avalue's customer services. To ensure you get the full benefit of our services, please follow the instructions below carefully.

Technical Support

We want you to get the maximum performance from your products. So if you run into technical difficulties, we are here to help. For the most frequently asked questions, you can easily find answers in your product documentation. These answers are normally a lot more detailed than the ones we can give over the phone. So please consult the user's manual first.

To receive the latest version of the user's manual; please visit our Web site at:

<http://www.avalue.com.tw/>

Content

- 1. Getting Started4**
 - 1.1 Safety Precautions4
 - 1.2 Packing List.....4
 - 1.3 System Specifications5
 - 1.4 System Overview7
 - 1.4.1 I/O View 7
 - 1.5 System Dimensions8
- 2. Hardware Configuration9**
 - 2.1 AID-173SHW connector mapping10
 - 2.1.1 Serial port 1 connector (COM1)..... 10
 - 2.1.2 Serial port 2 connector (COM2)..... 10

1. Getting Started

1.1 Safety Precautions

Warning!



Always completely disconnect the power cord from your chassis whenever you work with the hardware. Do not make connections while the power is on. Sensitive electronic components can be damaged by sudden power surges. Only experienced electronics personnel should open the PC chassis.

Caution!



Always ground yourself to remove any static charge before touching the CPU card. Modern electronic devices are very sensitive to static electric charges. As a safety precaution, use a grounding wrist strap at all times. Place all electronic components in a static-dissipative surface or static-shielded bag when they are not in the chassis.

1.2 Packing List

- 1 x AID-173SHW Medical PC
- 1 x Adapter
- 1 x Power cord



If any of the above items is damaged or missing, contact your retailer.

1.3 System Specifications

Component	
Mother Board	Proprietary and Custom Made
CPU	(1) Intel® Core™ i7-4650U Processor (4M Cache, up to 3.30 GHz) FC-BGA12F, Tray (2) Intel® Core™ i5-4300U Processor (3M Cache, up to 2.90 GHz) (3) Intel® Core™ i3-4010U Processor (3M Cache, 1.70 GHz)
CPU Cooler (Type)	Passive
Memory	DDR3L 1600 1 x SODIMM sockets Maximum 8GB Capacity
Power Supply	12 ~ 19V Wide Range Input
Adapter	60W 19V@3.15A IEC/EN 60601-1 Medical Adapter
System Fan	Fan-less
Microphone	1 x System Microphone
Speaker	2 x 2W High Quality System Speakers
Camera	1 x 2.0M Camera
Wireless LAN	Optional 1 x 802.11 b/g/n wireless LAN
Bluetooth	Optional External USB Bluetooth Dongle
Operating System	Win7/Win8/Linux
Other Component	SCR/MSR/RFID/Barcode Scanner / VOIP Handset
Storage	
Solid State Drive	1 x 2.5" 32G SATA SSD
Panel	
LCD Panel	17.3" TFT-LCD 1920*1080 from AUO / CMO-Innolux
LCD Control Board	LCD Built-in Inverter
B/L Inverter/Converter	LCD Built-in LED Backlight
Touch Screen	17.3" Projected Capacitive Touch Panel 17.3" Resistive Touch Panel
Touch Controller	Projected Capacitive Touch Controller Built-in Touch controller
External I/O	
Serial Port	1 x RS-232 1 x RS-232/422/485
USB Port	1 x USB 3.0 Port 3 x USB 2.0 Port


Video Port	1 x HDMI Input (Scalar Option) 1 x HDMI Output
Audio Port	1 x Earphone 1 x Mic
LAN Port	1 x RJ-45 LAN
Wireless LAN Antenna	2 x Built-In Wireless LAN Ant.
Switch	Capacitive Touch Button
Indicator Light	1 x Orange/Green LED Indicator (System) 1 x Green LED Indicator (Touch Button) 2 x Blue LED Indicators (Handset)
Expansion Slots	3 x Mini PCIe sockets 2 x full size (1 supports m-SATA) 1 x half size (USB only)
Mechanical	
Power Type	DC 12 ~ 19V
Power Connector Type	5.5 x 2.5 x 9.5 DC Jack
Dimension	448 (L) x 281 (H) x 45 (D) mm (w/o MSR/HS) 505(L) x 336 (H) x 51 (D) (w MSR/HS)
Weight	4.7Kgs
Color	White/Light Blue, Antimicrobial
Fan-less	Full System Fan-less
Reliability	
EMI Test	CE Class B, FCC Class B, MDD IEC/EN 60601-1
Safety	UL/IEC/EN 60601-1
Dust and Rain Test	IP-65 on Front Panel
Vibration Test	Standard(0.00454G ² /Hz,1.5Grms 5~500Hz)
Mechanical Shock Test	Standard
Drop Test	EC-60068-2-32 (96.5cm)
Operating Temperature	0 ~ 40C
Operating Humidity	10 ~ 90%
Storage Temperature	-20 ~ 60C



Note: Specifications are subject to change without notice.

1.4 System Overview


1.4.1 I/O View

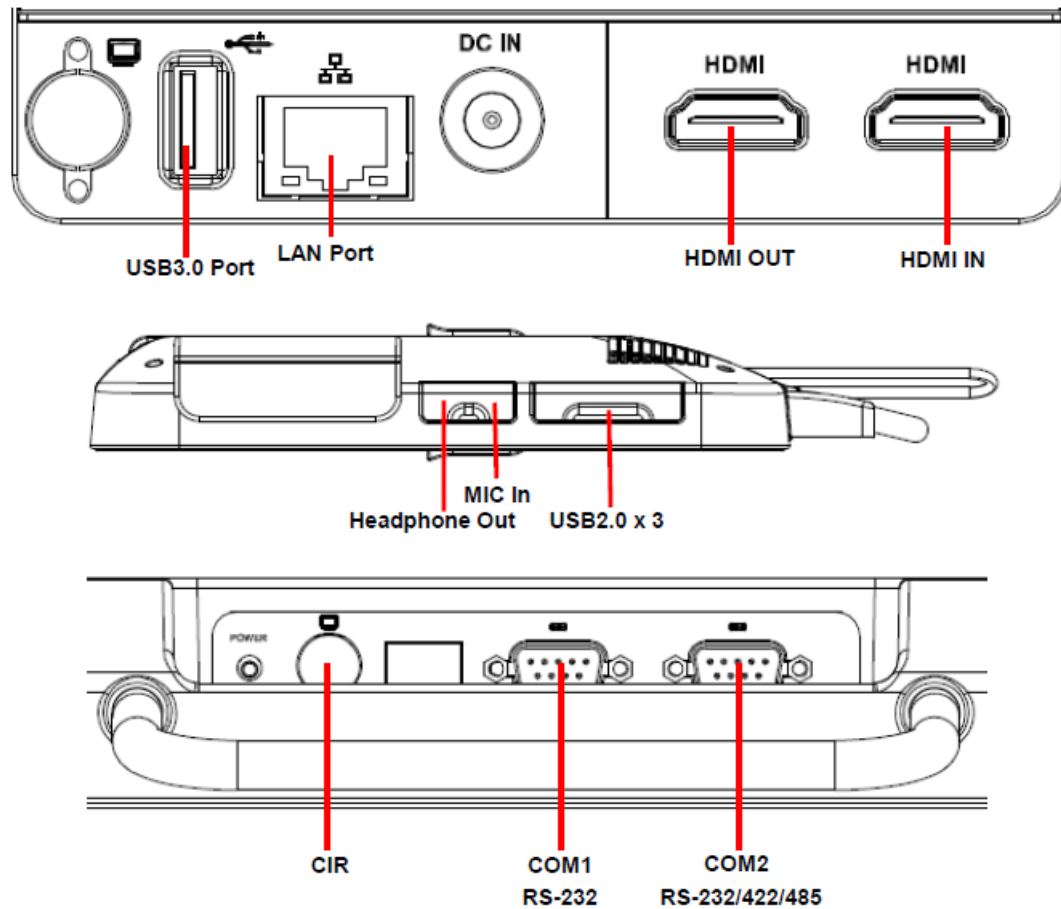

Connectors

Label	Function	Note
USB Port	3 x USB 2.0 connector 1 x USB 3.0 connector	
LAN Port	RJ-45 Ethernet connector	
COM1/2	Serial port 1/2 connector	DB-9 male connector Note : COM2 support RS422/485 by BIOS setting
HDMI IN	HDMI input connector	
HDMI OUT	HDMI output connector	
DC IN	connect to adapter	
MIC In	Mic-in audio jack	
Headphone Out	Line-out audio jack	
CIR	For IR cable (Optional)	

1.5 System Dimensions

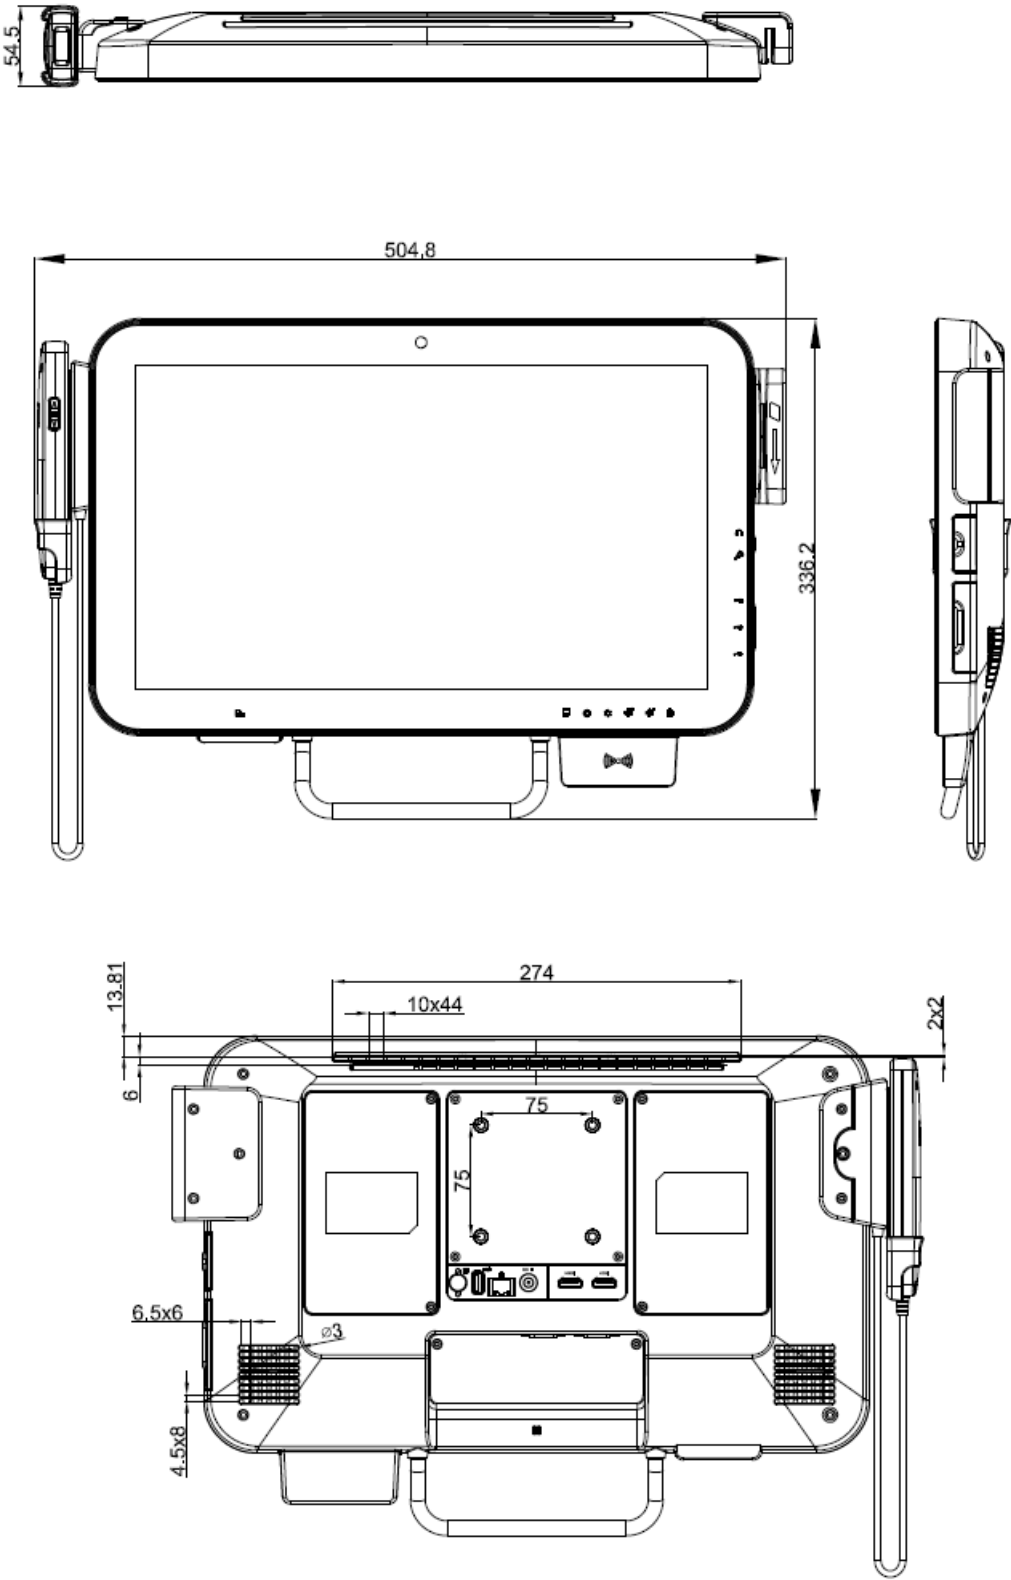

(Unit: mm)

2. Hardware Configuration





Note: If you need more information, please visit our website:

<http://www.avalue.com.tw>



2.1 AID-173SHW connector mapping

2.1.1 Serial port 1 connector (COM1)

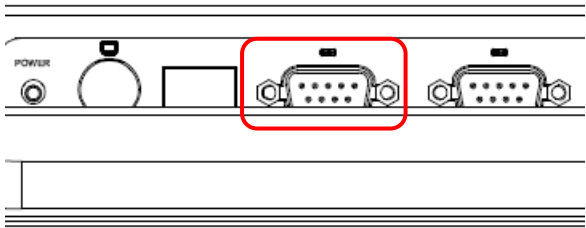

Signal	PIN	PIN	Signal
NDCD#	1	6	NDSR#
NRXD	2	7	NRTS#
NTXD	3	8	NCTS#
NDTR#	4	9	NRI#
GND	5		

2.1.2 Serial port 2 connector (COM2)

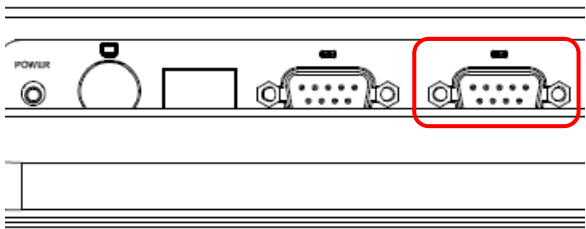

RS-232

Signal	PIN	PIN	Signal
DCD	1	6	DSR
RXD	2	7	RTS
TXD	3	8	CTS
DTR	4	9	RI
GND	5		

RS-485

Signal	PIN	PIN	Signal
DATA-	1	6	DATA+
NC	2	7	NC
NC	3	8	NC
NC	4	9	NC
GND	5		

RS-422

Signal	PIN	PIN	Signal
TxD-	1	6	TxD+
RxD+	2	7	NC
NC	3	8	RxD-
NC	4	9	NC
GND	5		

